


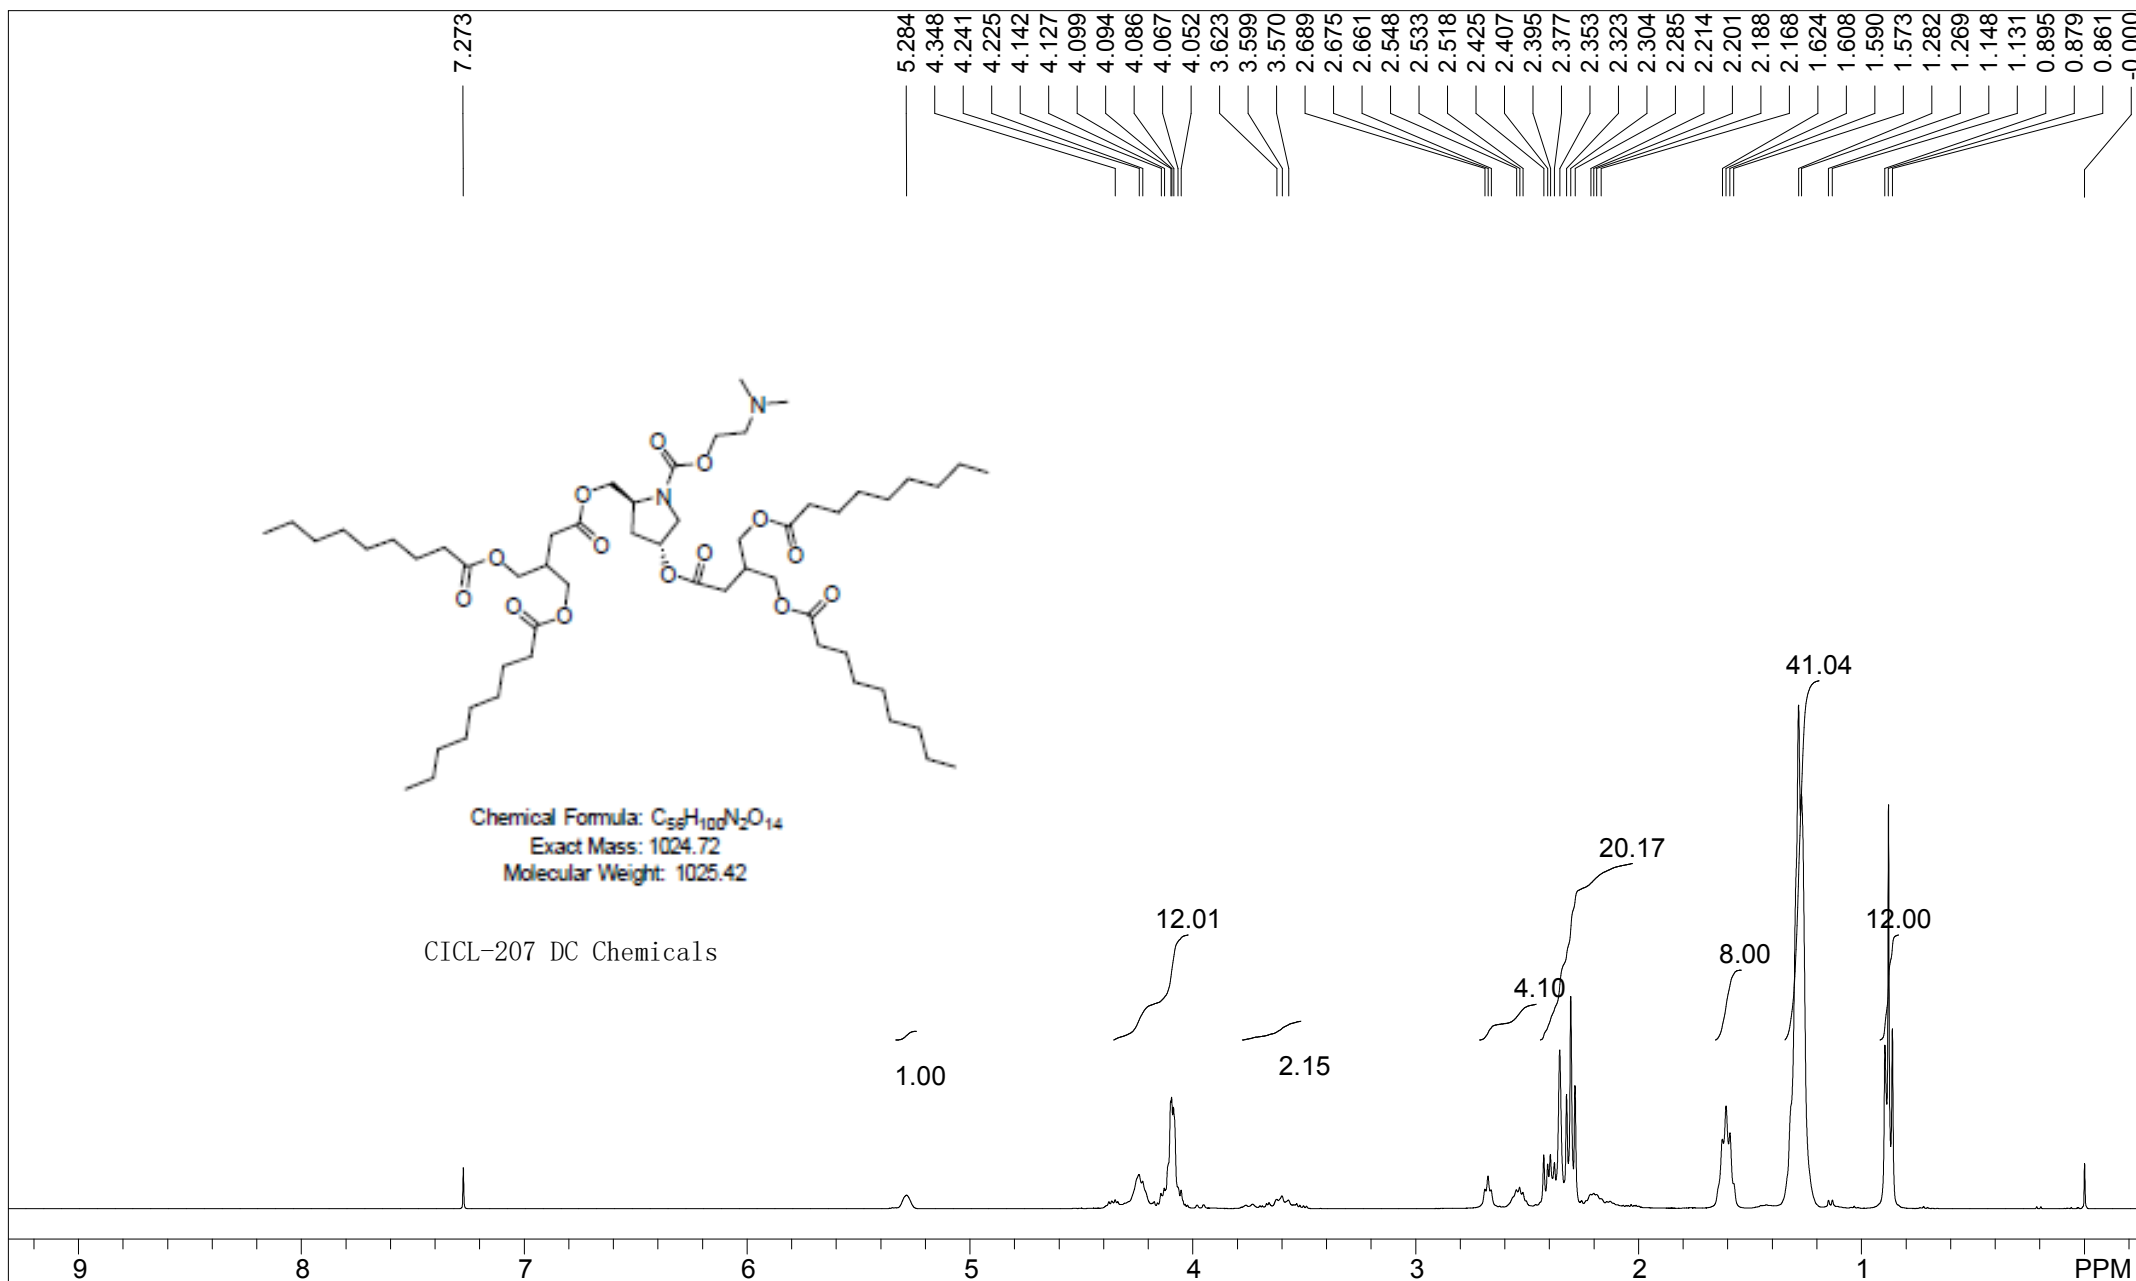

nmrB005, CDCl₃,

F1: 400.132

F2: 1.000

SW1: 8197

EX: zg30

PW: 8.0 usec

PD: 1.0 sec

OF1: 2466.6

NA: 8

LB: 0.0

USER: root -- DATE: Sat Sep 20 11:04:27 2025

PTS1d: 65536

Nuts - \$pdata

File D:\DATA\LCMS OF MS1024

Injection Date : 20 Sep 25 13:31 am +0800

Tgt Mass(EZX) :

Sample Name : LCMS OF MS1024

Location : P2-F-01

Acq. Operator : MONITOR

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 5 ul

Acq. Method : D:\METHODS\1-POS-3MIN-200-1800

Analysis Method : D:\METHODS\1-POS-3MIN-200-1800.M

Sample Info : Easy-Access Method: '1-POS-3MIN-200-1800'

Method Info : Mobile Phase: A: water (0.01% TFA) B: ACN (0.01% TFA)

Gradient: 5%B increase to 95%B within 1.3 min, 95%B for 1.7 min.


Flow Rate: 1.8 ml/ min

Column: Xbridge C8,4.6*50mm,3.5µm


Column Temperature: 45 °C

Detection:UV(214,4nm) and MS(ESI,Pos mode,110 to 1500 amu)


*ADC1 A, ELSD

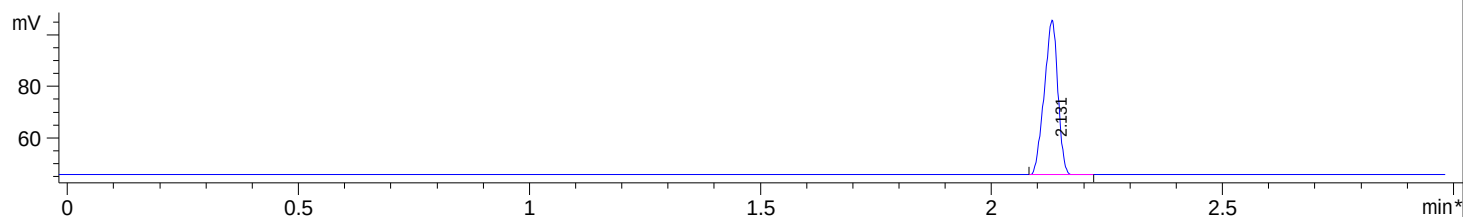


*DAD1 A, Sig=214,4 Ref=off

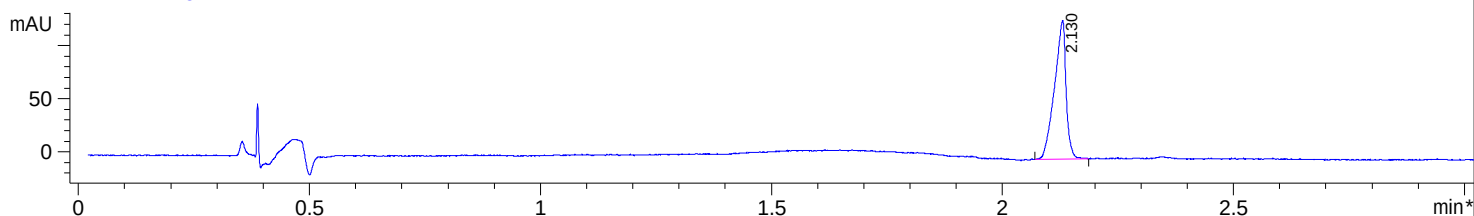

*DAD1 B, Sig=254,4 Ref=off

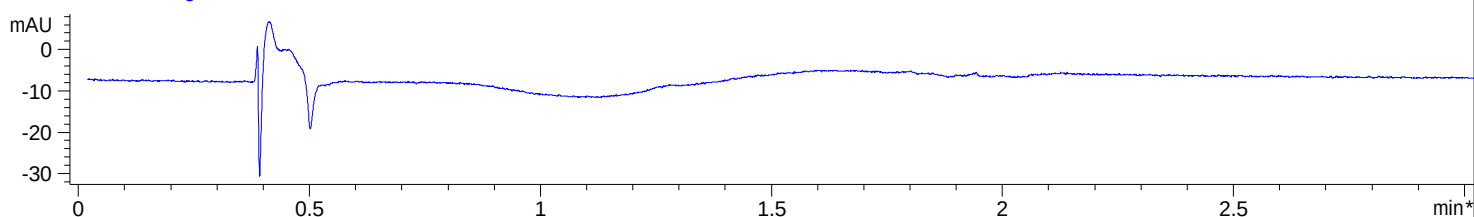

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

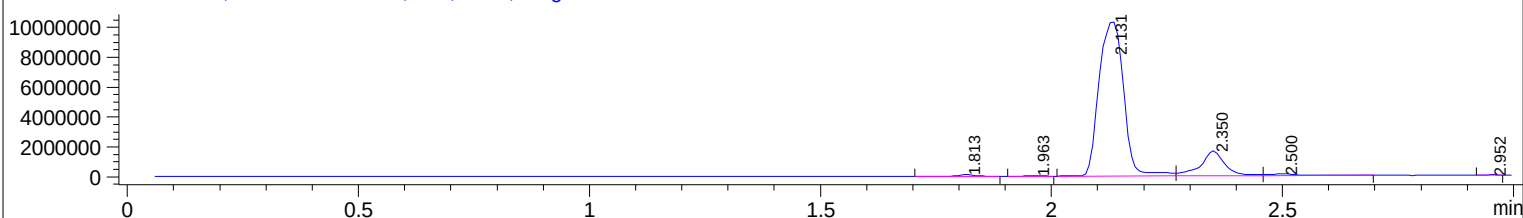

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
2.13	0.03	122.86	60.16	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
2.13	0.02	228.94	130.93	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%

Ret. Time: 1.81


<<<< POSITIVE SPECTRA >>>>

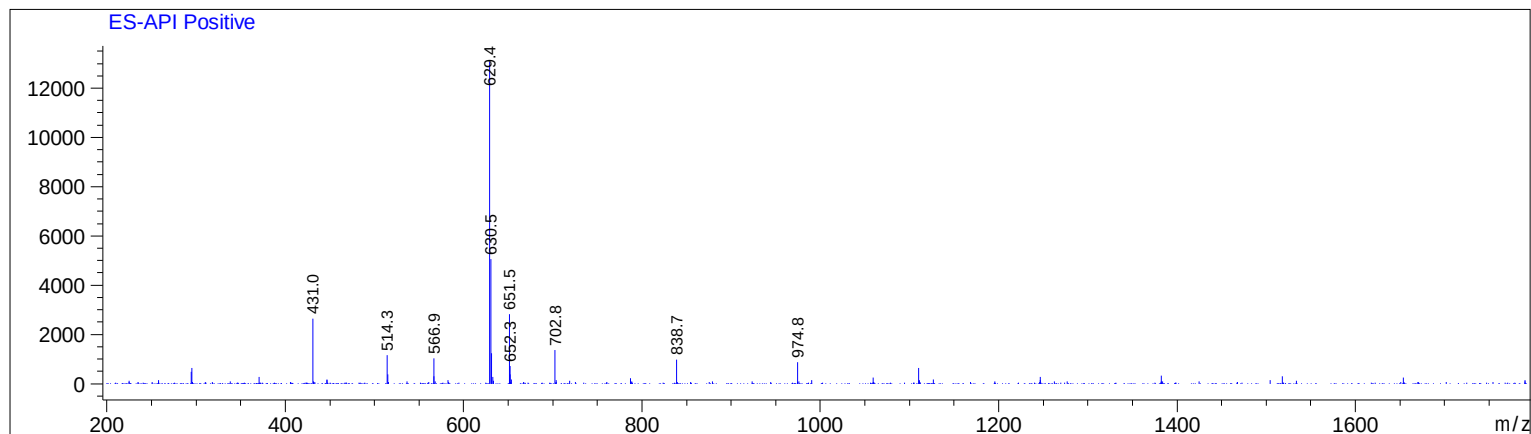


Ret. Time: 1.96

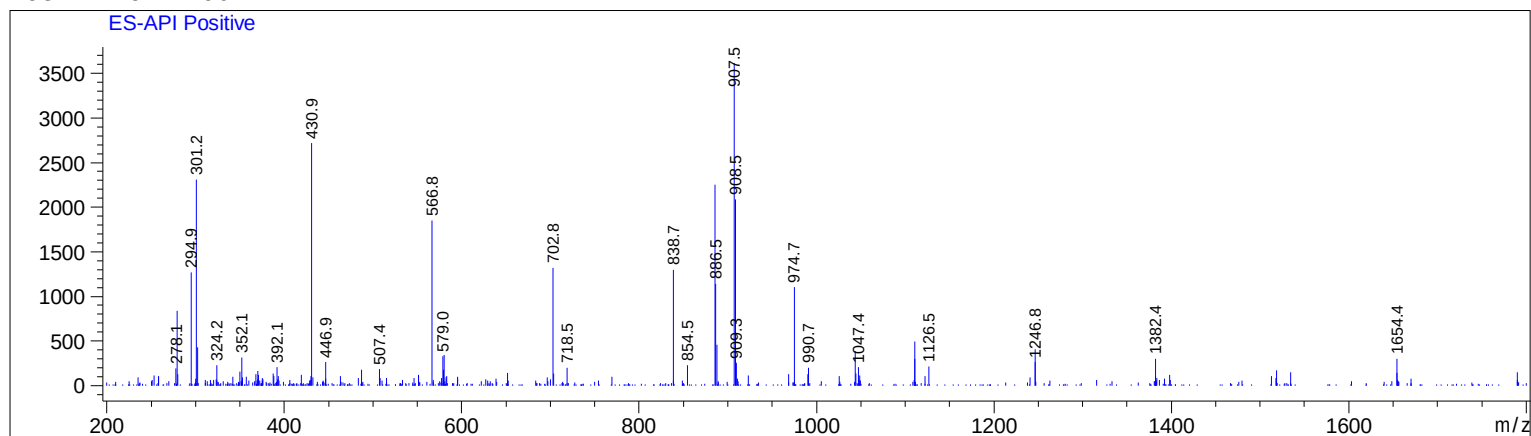


Ret. Time: 2.13

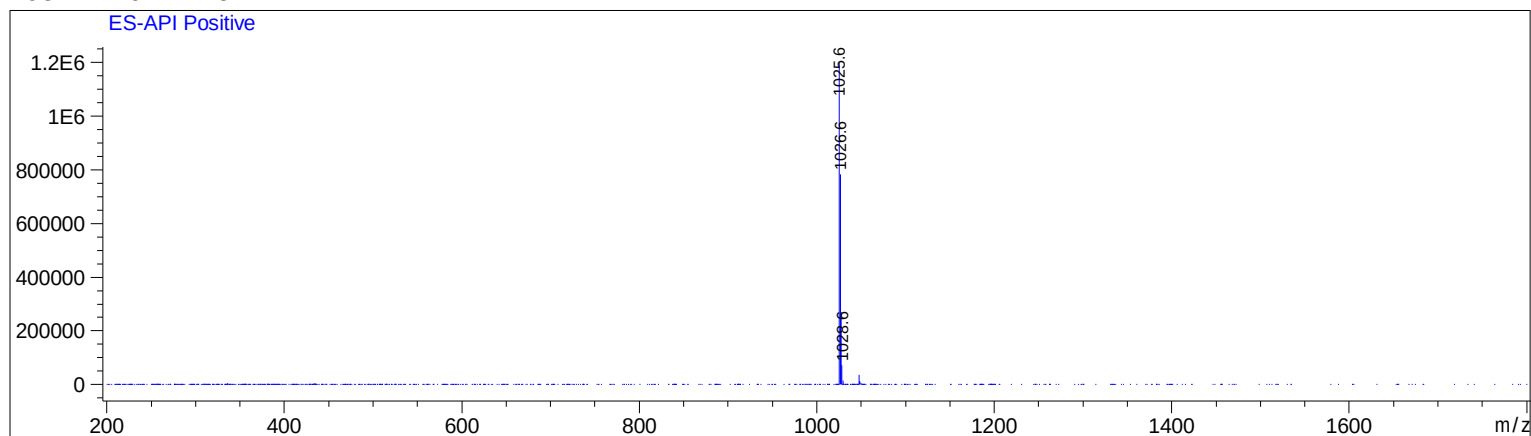

Ret. Time: 2.35

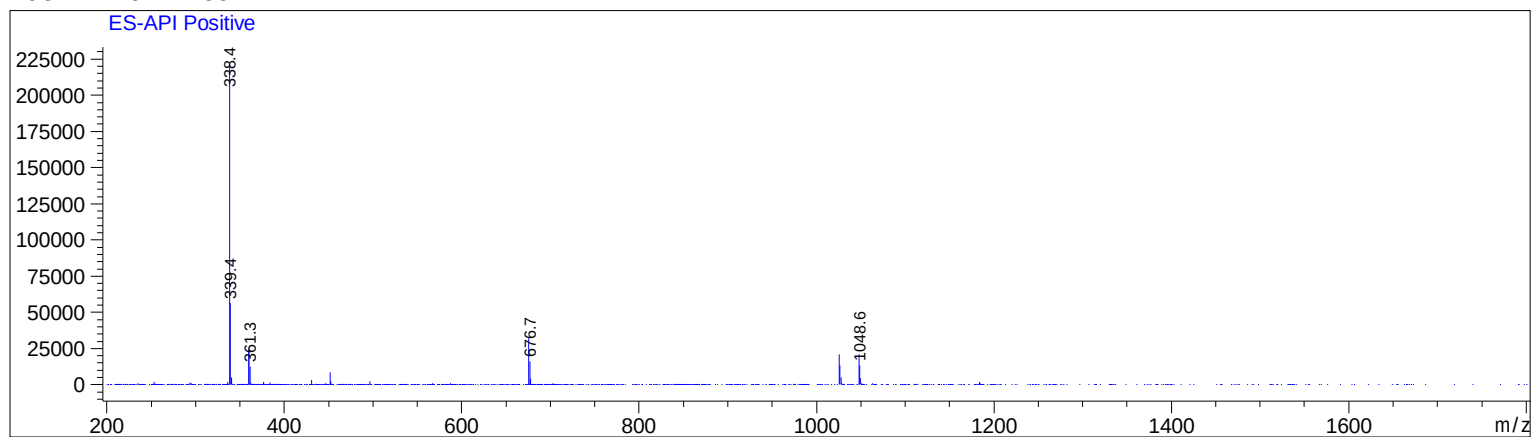

Ret. Time: 2.50

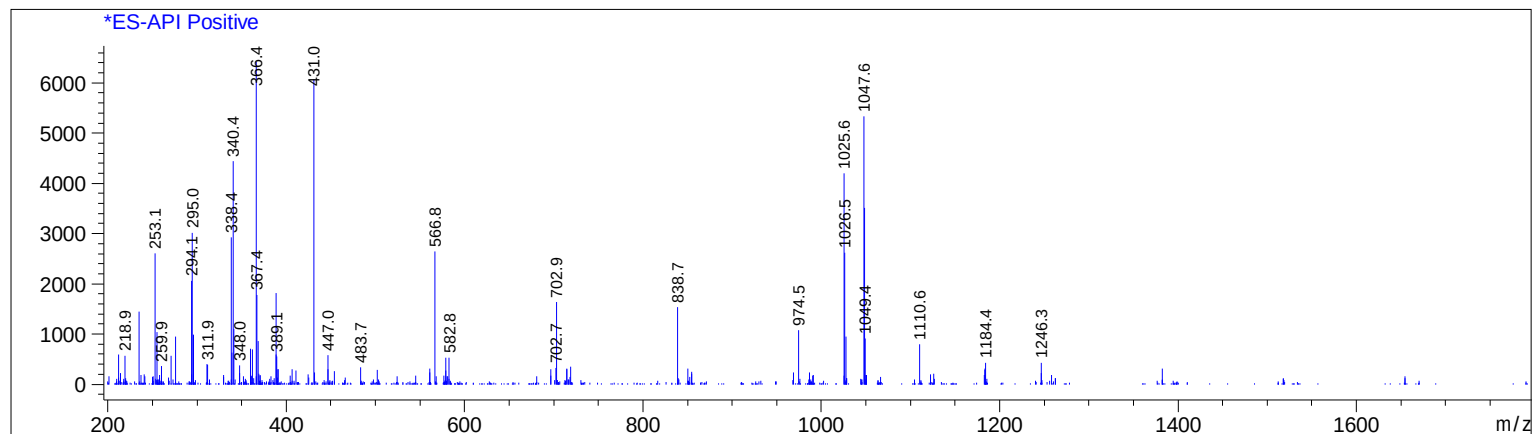

Ret. Time: 2.95

